


Radiographic measurement report

Horse: —

Study date: 2026-10-24

Calibration: 0.1869 mm/px (reference 55.0 mm)

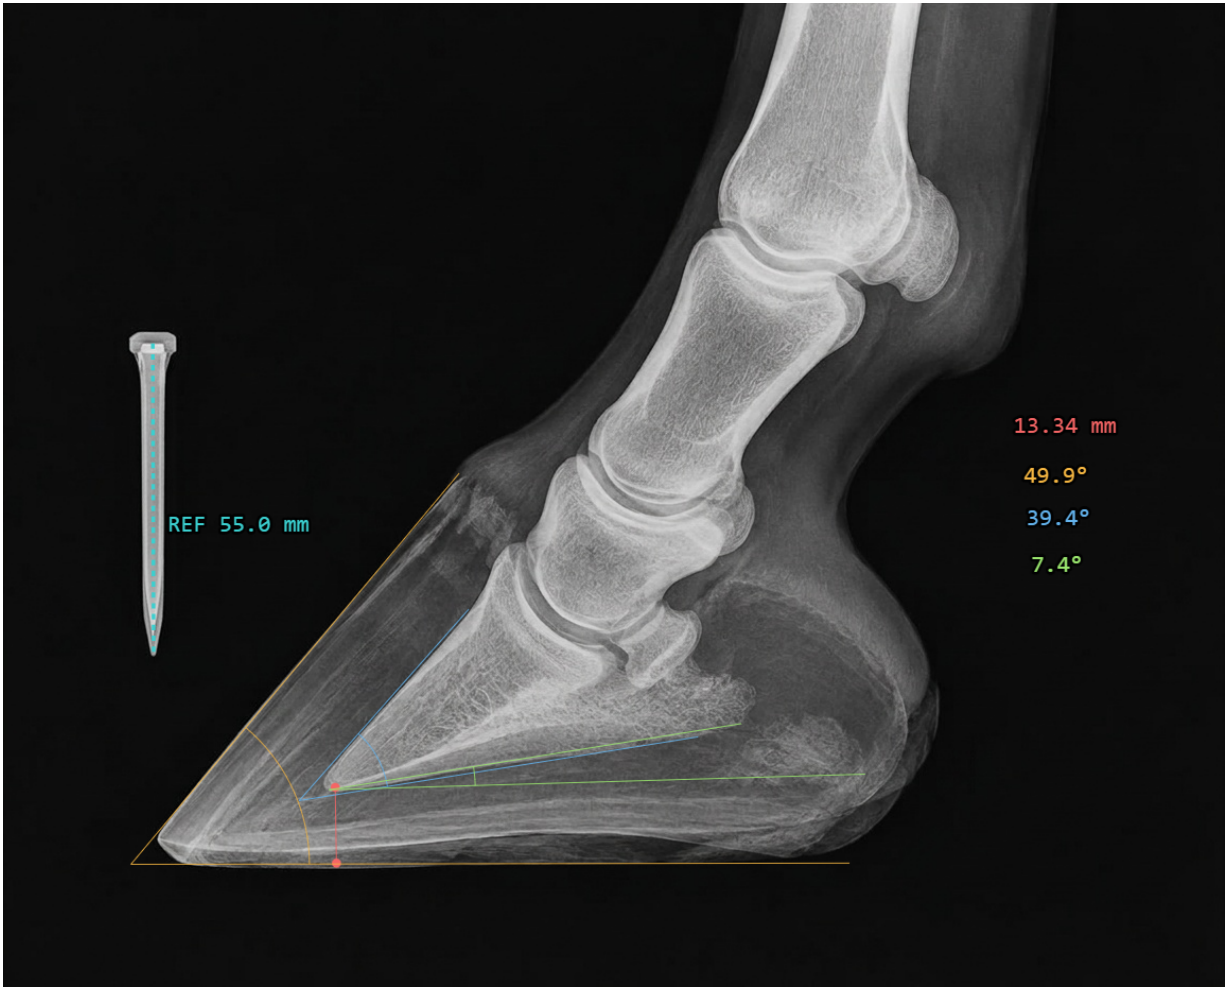

Measurements

SD	Distance	13.34 mm
HA	Three-point angle	49.87°
BA	Three-point angle	39.36°
PA	Three-point angle	7.44°

Distance accuracy requires the reference to be in the same plane as the structure (magnification/parallax).
These are geometric measurements; clinical interpretation is the responsibility of the practitioner.